

Facial iD[®] Orbital

Patient-specific orbital reconstruction implant

Envision **more**

Navigational markers and lines

work with Q Guidance, Nav3i, Scopis or your preferred navigation system

Solid, mesh or hybrid designs


to meet your reconstructive needs

Personalized design

made of 3D printed, commercially pure titanium

Multiple thicknesses

0.3mm, 0.6mm, 0.9mm

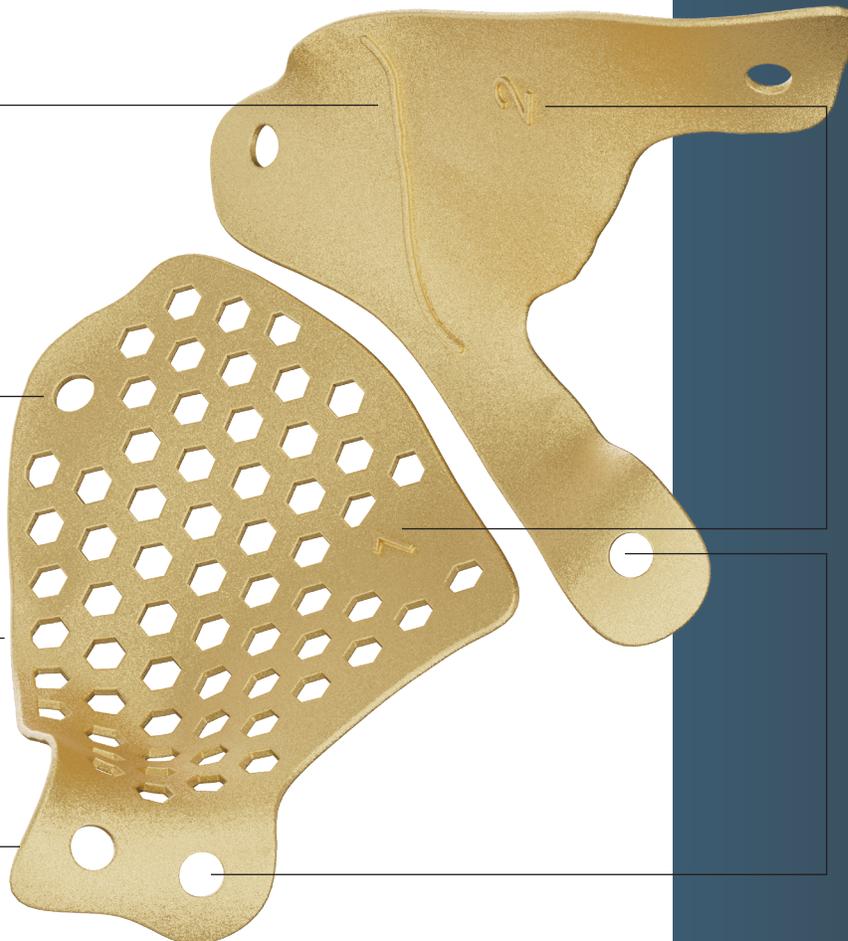

Implant identification numbers

denote multi-piece designs

You choose screw location;

position on implant surface or as extension arm

Surgeon driven design


Facial iD Orbital implants **save OR time** vs stock¹

Facial iD Orbital implants can provide a **more accurate fit** vs stock²

SSM provides an **accurate reconstruction surface** for orbital repair³

Stryker's exclusive orbital statistical shape modeling

Facial iD Orbital launches with a dedicated orbital reconstruction software designed with our proprietary statistical shape model. SSM utilizes 100+ CT scans of males and females ages 15-99 from a variety of ethnicities to provide a normative orbital model as a foundation for implant design.³

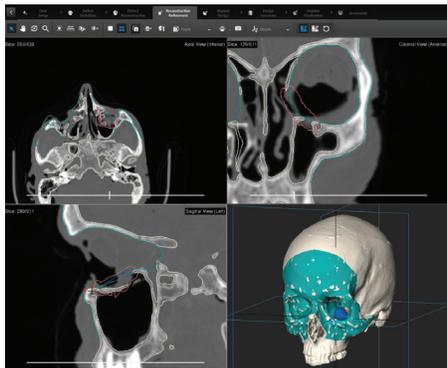

◀ During the virtual design session that model is seamlessly blended with the patient's native anatomy to create an idealized planning surface independent of the contralateral side. The implant surface can be modified and adjusted based on your preferences and patient needs.



1. Due to less intraoperative bending; Data on file at Stryker
2. Due to patient-specific nature and design to patient CT; Data on file at Stryker
3. Data on file at Stryker

Craniomaxillofacial

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of specific products before using them in surgery.

The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker or its affiliated entities own, use, or have applied for the following trademarks or service marks: Facial iD, Nav3i, Q Guidance, Scopis and Stryker. All other trademarks are trademarks of their respective owners or holders.

Stryker
1941 Stryker Way
Portage, MI 49002 USA
t: 269 389 5346 f: 800 962 6558
toll free: 877 648 7114

stryker.com