


Pediatric Mandibular Distractor


with anti-reverse mechanism

Clockwise turn

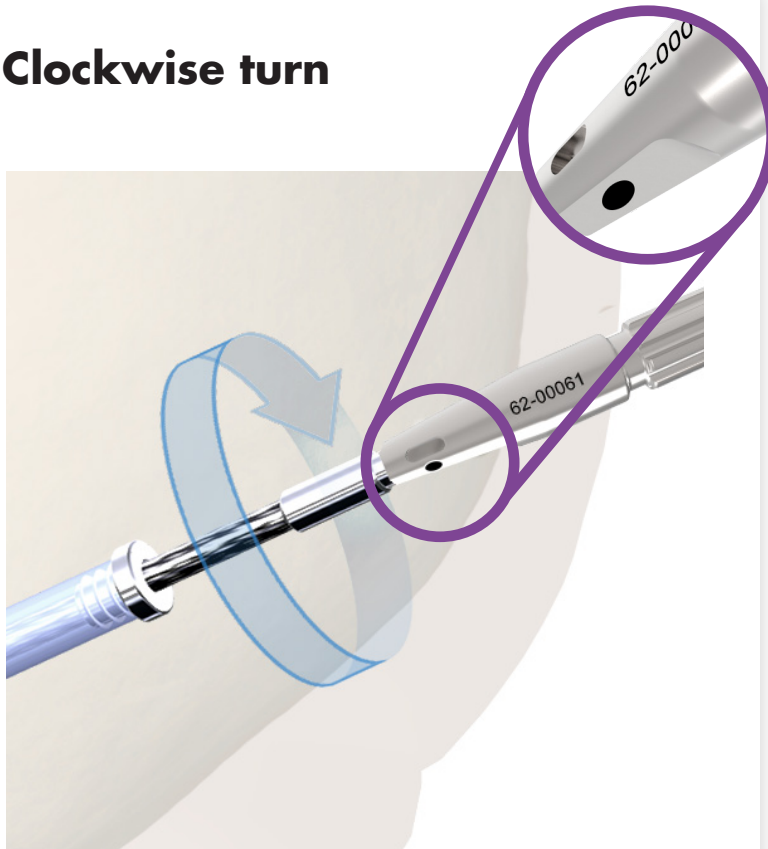

- To execute a full 360° clockwise turn, the **black dot on the activation handle** should return back to its original position

One 360° turn = 0.5mm of advancement

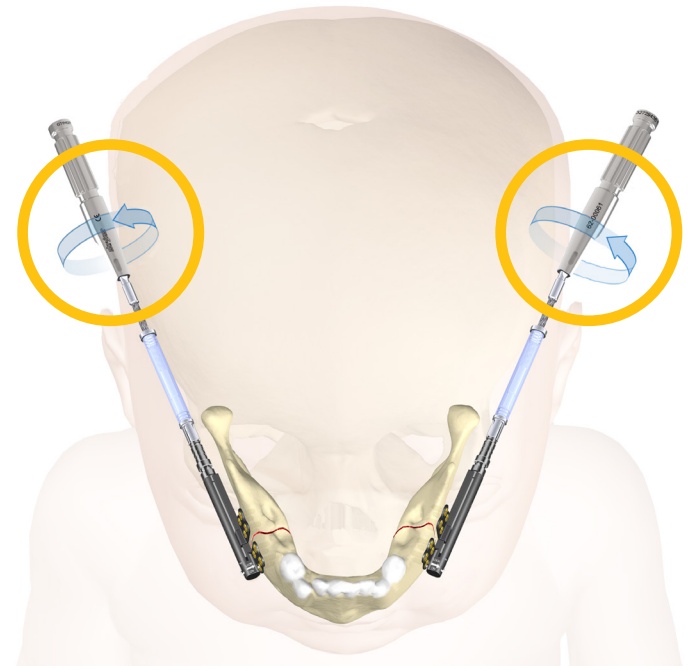

- When the activation handle is attached to the activation rod(s), **only turn the handle in the clockwise direction**

