


**stryker**



# AlphaVent

**Versatile. Strong. Confidence in every repair.**

Hard-body, screw-in  
anchor platform

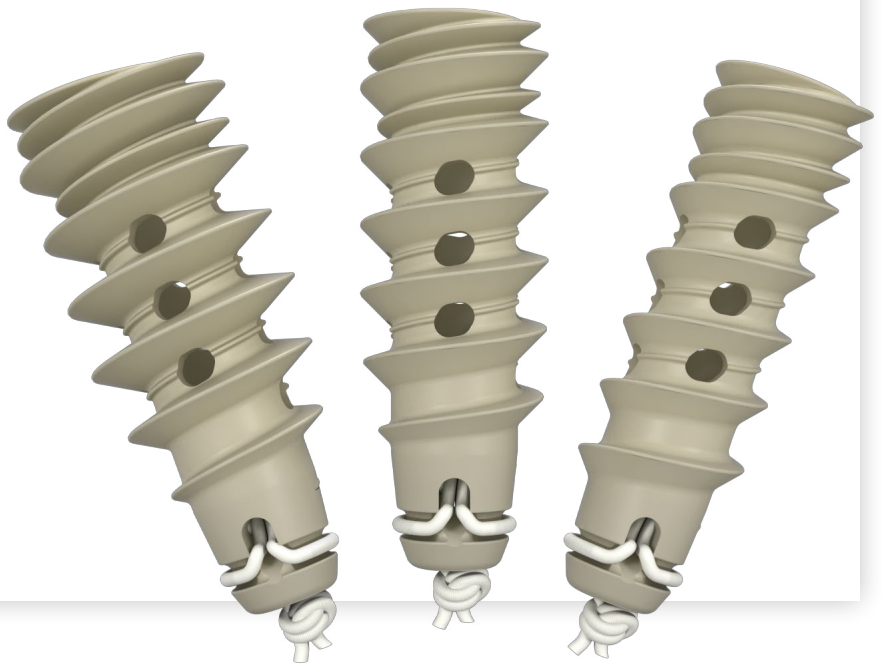

6.5mm


5.5mm

4.75mm

# Designed to perform


## Proprietary soft triple eyelet

- **Higher strength** than eyelets of leading competitors' anchors<sup>1</sup>
- Accommodates sliding and non-sliding sutures
- Facilitates smooth suture sliding

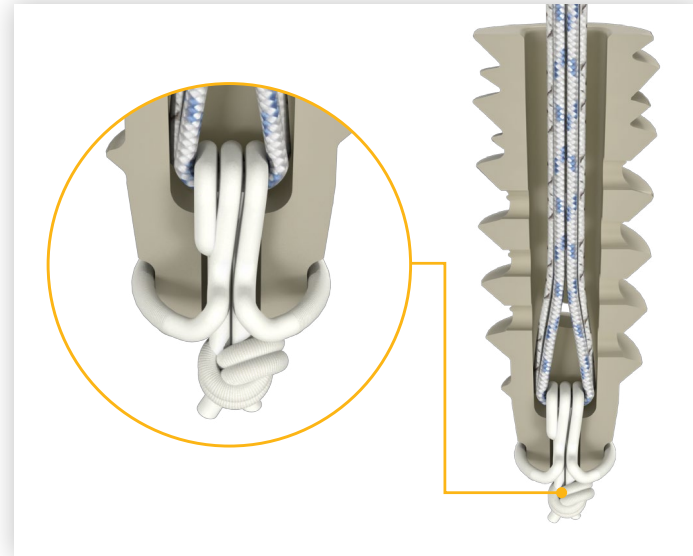

## Dual-thread technology

- Devised to improve anchor performance through optimized engagement in cortical and cancellous bone<sup>1</sup>
- Provides tactile feedback during cortical thread engagement

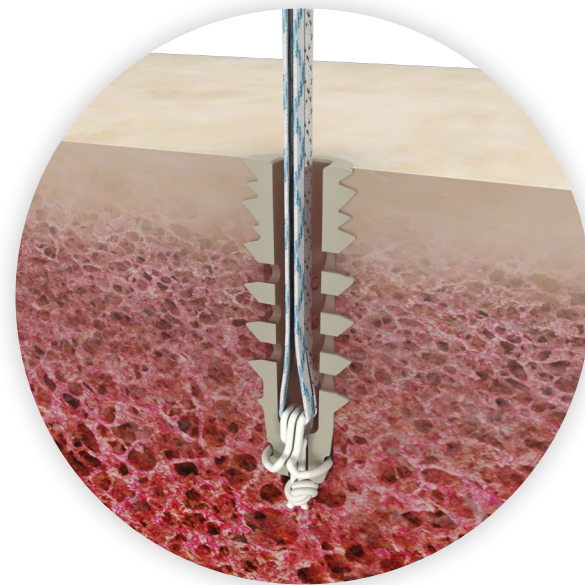


## Unobstructed cannulation meets complete venting

- Allows exchange of blood and other autologous cells at the healing site


# Versatile platform

Designed to comprehensively meet procedural and surgical technique needs:

- Three anchor sizes
- Ten different high-strength UHMWPE suture configurations
- Sliding and non-sliding sutures
- Needled and non-needed options
- Instrumentation for all bone qualities

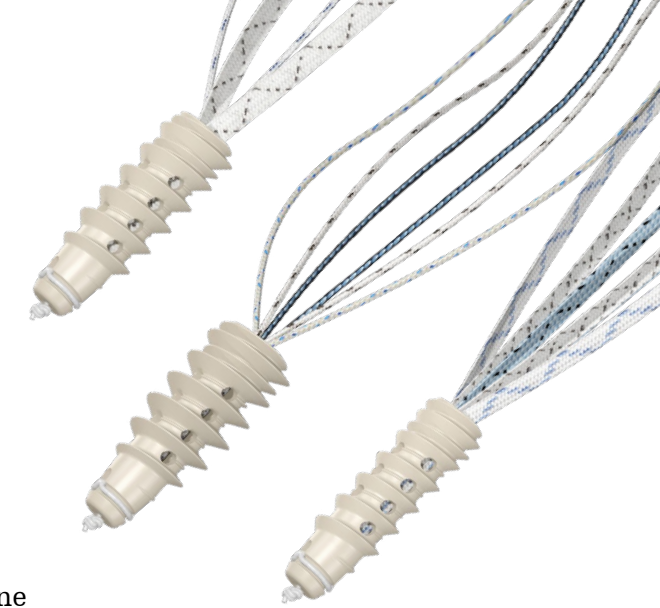

**Needles safely stored** in handle for relevant configurations

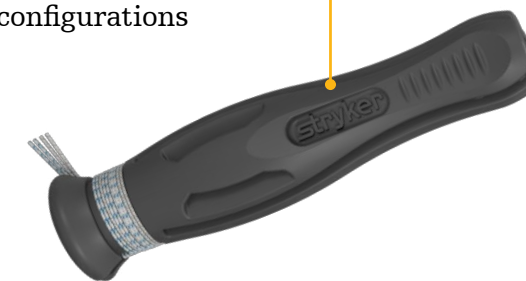

**Fully slotted driver** allows for intraoperative screw re-engagement and removal

**16mm length** allows for multiple points of fixation without screw convergence in double-row repairs

**Tapered tip** facilitates ease of insertion



## Instrumentation for all bone qualities

- Variety of instruments for appropriate pilot hole creation
- Conveniently, offered both sterile and non-sterile to meet customer and facility needs



AlphaVent delivers the options you need and the strength you expect **for confidence in every repair.**

**Product number Description**

**5.5mm suture anchors**

3910955022	5.5mm suture anchor, PEEK, 2 strands of #2 Force Fiber
3910955032	5.5mm suture anchor, PEEK, 3 strands of #2 Force Fiber
3910955132	5.5mm suture anchor, PEEK, 3 strands of #2 Force Fiber with needles
3910955021	5.5mm suture anchor, PEEK, 2 strands of 1.4mm XBraid TT
3910955031	5.5mm suture anchor, PEEK, 3 strands of 1.4mm XBraid TT
3910955020	5.5mm suture anchor, PEEK, 2 strands of 1.8mm XBraid TT
3910955221	5.5mm suture anchor, PEEK, 1 strand of 1.8mm XBraid TT and 1 strand of 1.4mm XBraid TT
3910955222	5.5mm suture anchor, PEEK, 1 strand of 1.8mm XBraid TT and 1 strand of #2 Force Fiber

**6.5mm suture anchors**

3910965032	6.5mm suture anchor, PEEK, 3 strands of #2 Force Fiber
3910965031	6.5mm suture anchor, PEEK, 3 strands of 1.4mm XBraid TT
3910965221	6.5mm suture anchor, PEEK, 1 strand of 1.8mm XBraid TT and 1 strand of 1.4mm XBraid TT
3910965222	6.5mm suture anchor, PEEK, 1 strand of 1.8mm XBraid TT and 1 strand of #2 Force Fiber

**Instrumentation**

3910947200	3.9mm Omega and 4.75mm AlphaVent Awl
3910947201	4.75mm AlphaVent and Omega Awl
3910947202	4.75mm AlphaVent and Omega Drill
3910947207	4.75mm AlphaVent Tap
3910947208	4.75mm AlphaVent Punch-Tap
3910947203	5.5mm AlphaVent and 4.75mm Hard Bone Omega Drill
3910947209	5.5mm AlphaVent Tap
3910947212	Drill Guide

**Product number Description**

**4.75mm suture anchors**

3910947022	4.75mm suture anchor, PEEK, 2 strands of #2 Force Fiber
3910947032	4.75mm suture anchor, PEEK, 3 strands of #2 Force Fiber
3910947132	4.75mm suture anchor, PEEK, 3 strands of #2 Force Fiber with needles
3910947021	4.75mm suture anchor, PEEK, 2 strands of 1.4mm XBraid TT
3910947031	4.75mm suture anchor, PEEK, 3 strands of 1.4mm XBraid TT
3910947131	4.75mm suture anchor, PEEK, 3 strands of 1.4mm XBraid TT with needles
3910947020	4.75mm suture anchor, PEEK, 2 strands of 1.8mm XBraid TT
3910947120	4.75mm suture anchor, PEEK, 2 strands of 1.8mm XBraid TT with needles
3910947221	4.75mm suture anchor, PEEK, 1 strand of 1.8mm XBraid TT and 1 strand of 1.4mm XBraid TT
3910947222	4.75mm suture anchor, PEEK, 1 strand of 1.8mm XBraid TT and 1 strand of #2 Force Fiber

**References:**

1. DHD14695, TR21098

**Sports Medicine**

This document is intended solely for the use of healthcare professionals. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. We do not dispense medical advice and recommend that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate Stryker's products. A surgeon must always refer to the package insert, product label and/or instructions for use, including the instructions for cleaning and sterilization (if applicable), before using any of Stryker's products. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets.

Please contact your representative if you have questions about the availability of Stryker's products in your area.

Stryker or its affiliated entities own, use, or have applied for the following trademarks or service marks: AlphaVent, XBraid, Force Fiber, Omega, PEEK and Stryker. All other trademarks are trademarks of their respective owners or holders.

The absence of a product, feature, or service name, or logo from this list does not constitute a waiver of Stryker's trademark or other intellectual property rights concerning that name or logo.

1000904064 Rev B

Copyright © 2021 Stryker

Stryker  
Sports Medicine  
5670 Greenwood Plaza Blvd.  
Ste. 200  
Greenwood Village, CO 80111  
t: 866 596 2022  
www.sportsmedicine.stryker.com